


ANAESTHETICS

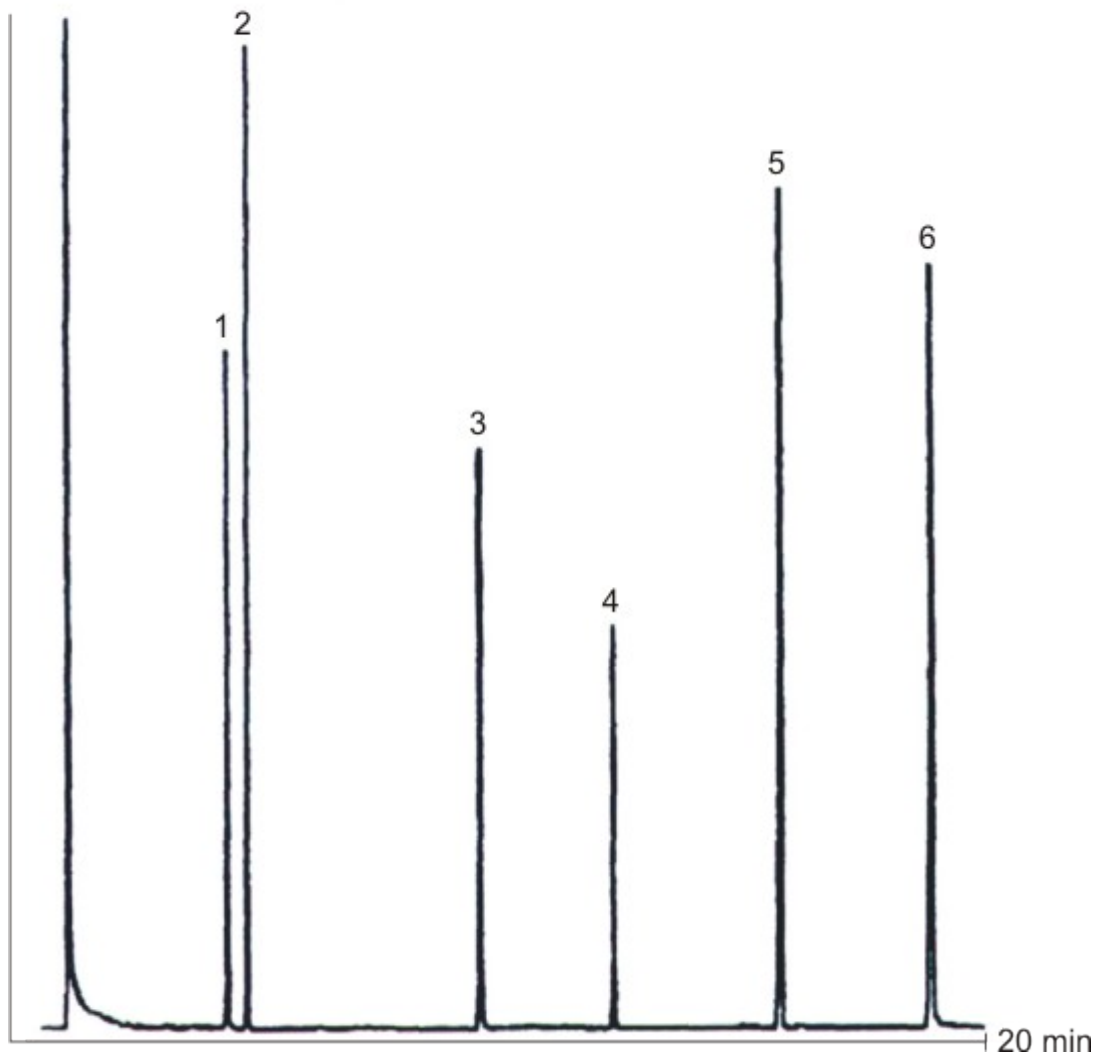

Column

Phase	MEGA-5
I.D.	0.25 mm
Film Thickness	0.25 µm
Length	25 m

Chromatographic Conditions

Injection	Split	280°C
Split Ratio	1:70	
Injection volume	0.5 µL	
Oven	T start	150°C
	Rate	5°C/min
	T end	250°C
Detector	FID	250°C
Carrier Gas	Hydrogen	60 kPa

Peak Identification

1	Benzocaine
2	Amilocaine
3	Lidocaine
4	Procaine
5	Cocaine
6	Codeine