


AROMES (TEST MIXTURE)

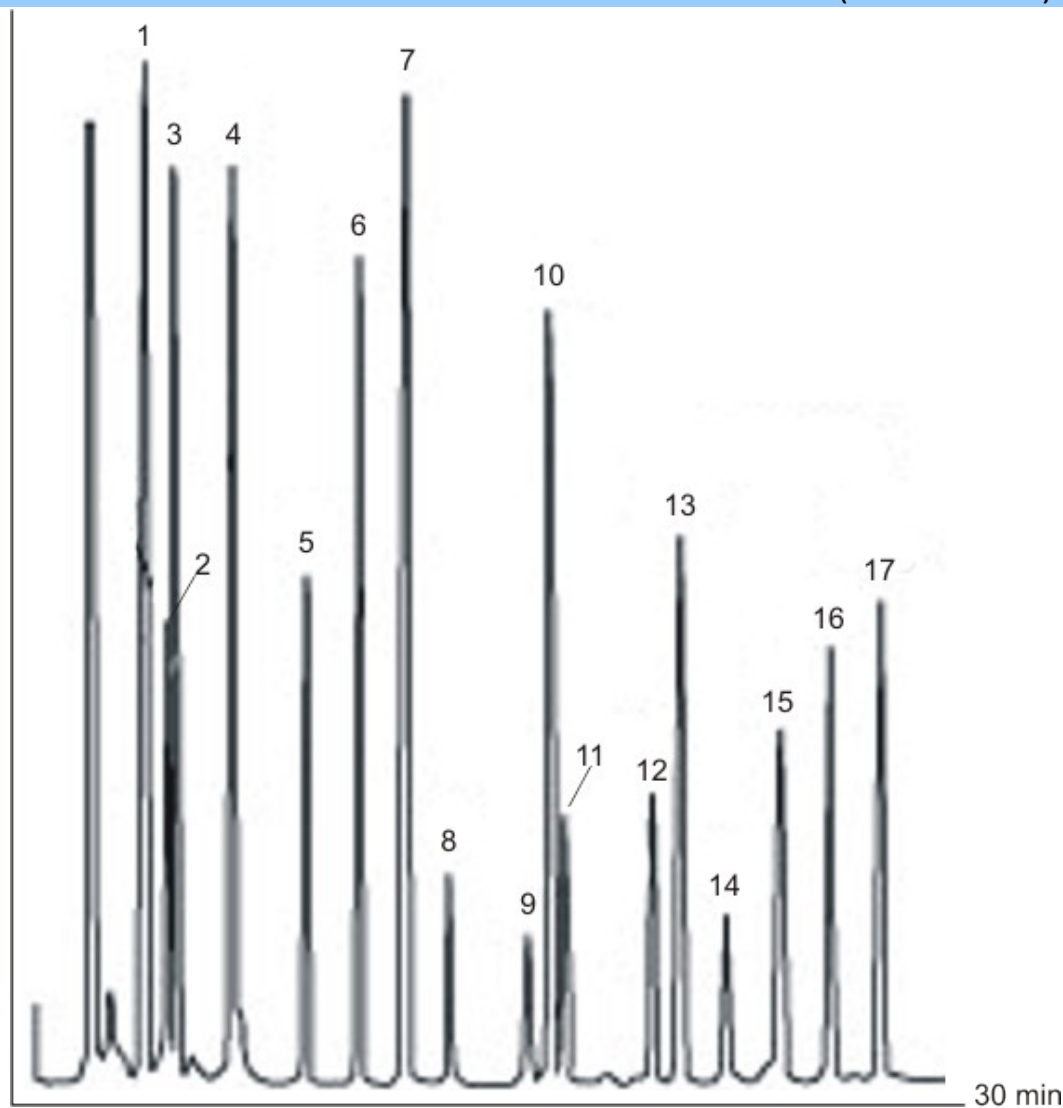

Column

Phase	MEGA-ACID
I.D.	0.25 mm
Film Thickness	0.25 µm
Length	25 m

Chromatographic Conditions

Injetor	Split	
Oven	T start	75°C
	Rate	2°C/min
	T end	140°C
Detector	FID	
Carrier Gas	Helium	1.7 mL/min

Peak Identification

1	Isoamyl acetate
2	α-Phellandrene
3	Cumene
4	1-Pentanol
5	6-Methyl,5-Hepten,2-one
6	2-Nonanone
7	Ethyl Octanoate
8	Furfural
9	Benzaldehyde
10	Linalool
11	Isobutyric Acid
12	n-Butyric Acid
13	Ethyl Decanoate
14	Furfuryl Alcohol
15	α + β Terpineol
16	Carvone
17	Methyl Salicylate