


BERGAMOT

Courtesy Prof. C. Bicchi, C. Brunelli – Università di Torino, Dipartimento Scienza e Tecnologia del Farmaco –
Via P.Giuria, 9 – Torino

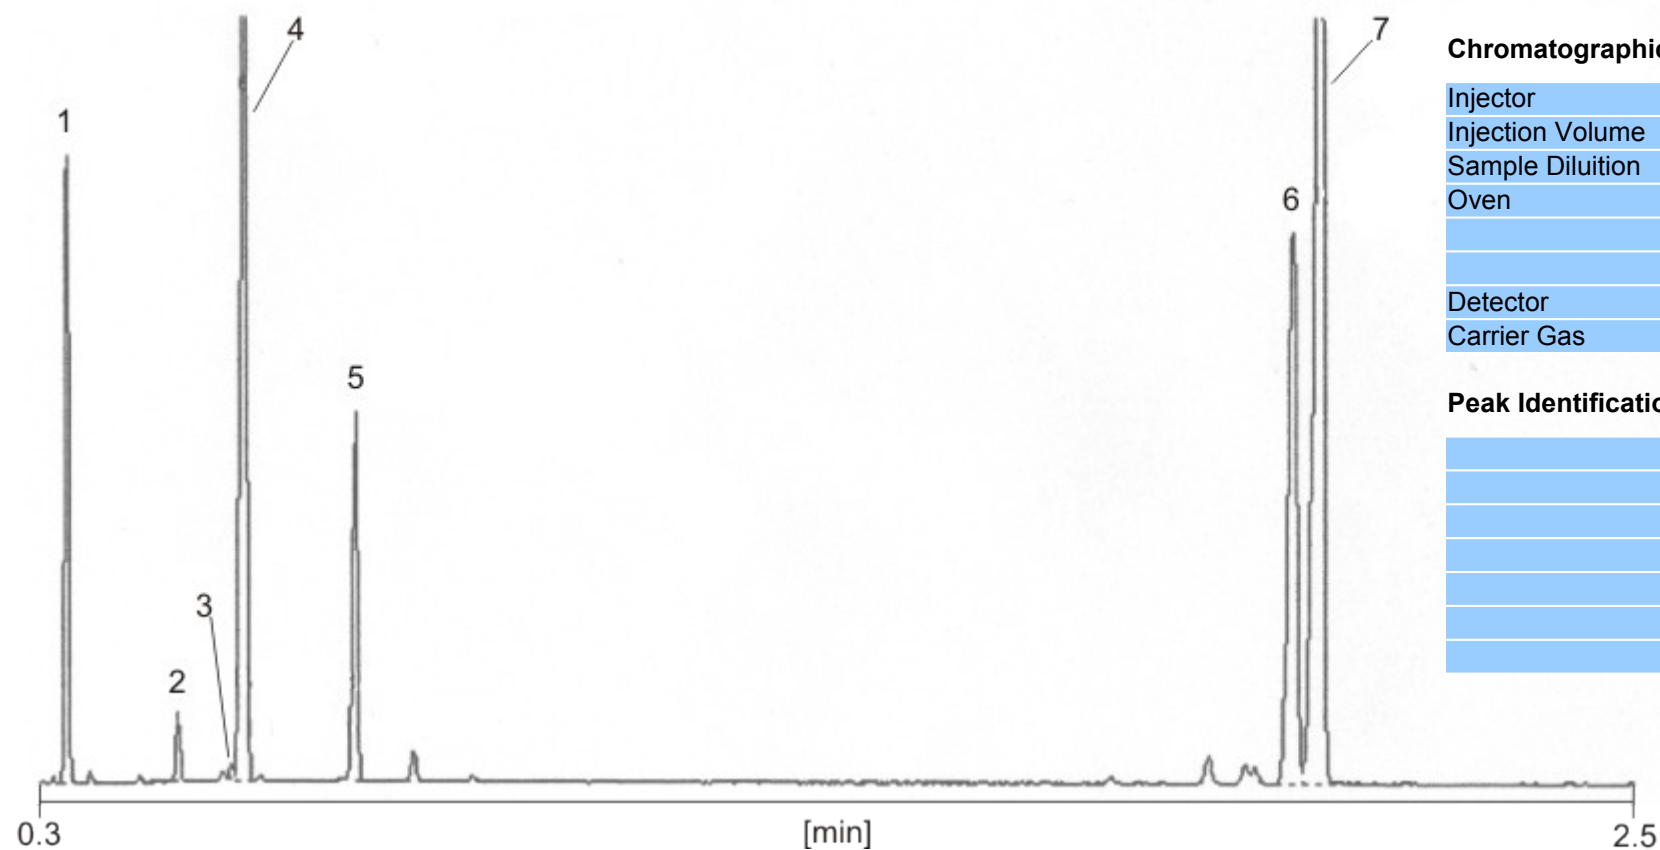

Column

Phase	MEGA-WAX
I.D.	0.1 mm
Film Thickness	0.1 µm
Length	5 m

Chromatographic Conditions

Injector	Split	230°C
Injection Volume	1.0 µL	
Sample Dilution	1:200	in Cyclohexane
Oven	T start	50°C (0.1 min)
	Rate	30°C/min
	T end	250°C (5 min)
Detector	FID	250°C
Carrier Gas	Hydrogen	0.5 mL/min

Peak Identification

1	β-Pinene
2	Myrcene
3	p-Cimene
4	Limonene
5	γ-Terpinene
6	Linalool
7	Linalyl Acetate