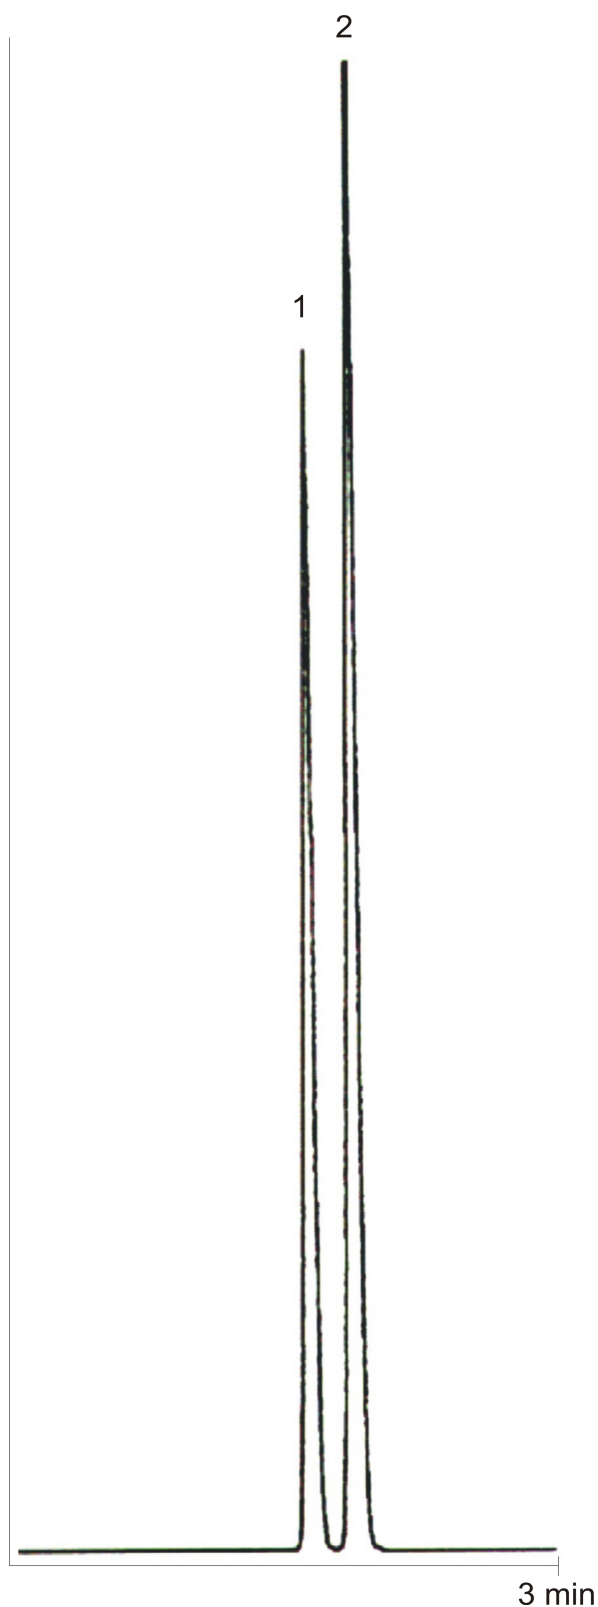


GAS ANAESTHETICS**Column**

Phase	MEGA-PS264
I.D.	0.32 mm
Film Thickness	5 µm
Length	30 m

Chromatographic Conditions

Injector	Split	250°C
Split Ratio	1:50	
Injection Volume	10 µL	
Oven	Isot.	40°C
Detector	FID	250°C
Carrier Gas	Hydrogen	40 kPa

Peak Identification

1	Isoflurane
2	Enflurane