


**Halogenated Volatiles**  
**EPA Method 551**  
on MEGA-VOC 1 column (USP G43 phase)

Column: **MEGA-VOC 1 - 0.25mm, 1.40µm, 30m**  
Catalog Code: C-VOC1-025-140-30

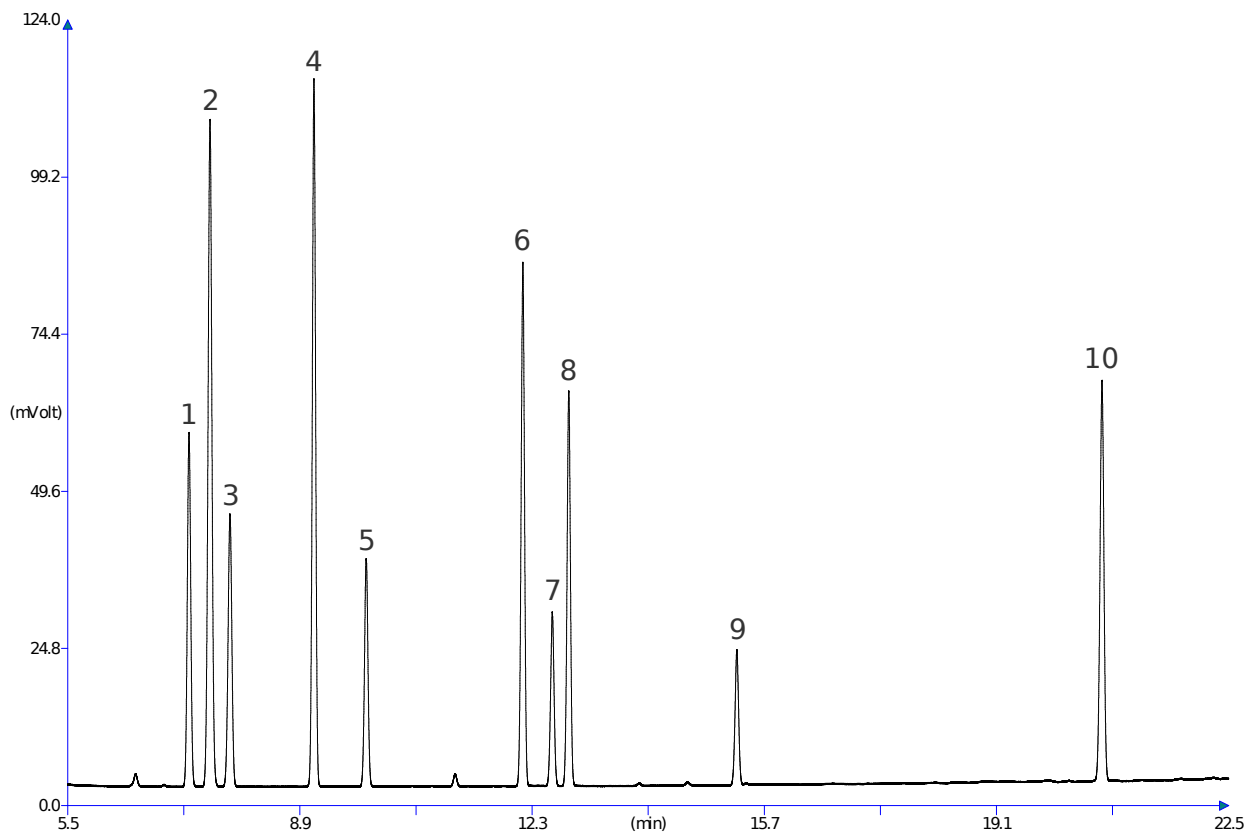

**Conditions:**

Injection: Split, 250°C, 2µL, 30mL/min Split Flow.

Sample: 2000µg/mL each in Acetone.

Detector: FID, 285°C.

Oven Temp.: 40°C (2min), 8°C/min, 210°C.

Carrier Gas: Helium, 85 kPa.

**Peaks:**

1. Chloroform
2. 1,1,1-Trichloroethane
3. Carbon tetrachloride
4. Trichloroethylene
5. Bromodichloromethane
6. Tetrachloroethylene
7. Dibromochloromethane
8. 1,2-Dibromoethane
9. Bromoform
10. 1,2-Dibromo-3-chloropropane

